

1. PERFORMANCE


- 1) Measuring range : 0.1-1.0 %
Number of pump strokes : 1 (100mℓ)
- 2) Sampling time : 0.5 minutes/ 1 pump stroke
- 3) Detectable limit : 0.01 %
- 4) Shelf life : 2 years
- 5) Operating temperature : 0 ~ 40℃
- 6) Reading : Direct reading from the scale calibrated by 1 pump stroke
- 7) Colour change : Pale purple → Pale yellow

2. RELATIVE STANDARD DEVIATION

RSD-low : 5 % RSD-mid : 5 % RSD-high : 5 %

3. CHEMICAL REACTION

By reacting with Phosphoric acid, PH indicator is discoloured.



4. CALIBRATION OF THE TUBE

STANDARD GAS CYLINDER METHOD

5. INTERFERENCE AND CROSS SENSITIVITY

Substance	Interference	ppm	Coexistence
Amines FIG.1	Similar stain is produced.		Higher readings are given.
Sulphur dioxide	The accuracy of readings is not affected.	200	Lower readings are given.

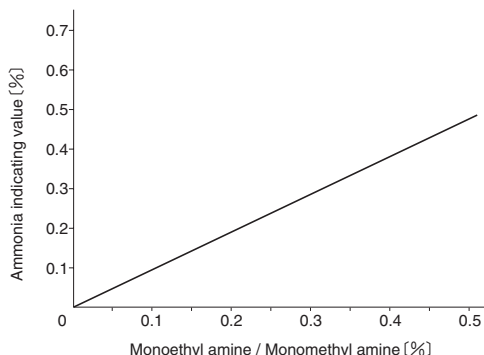


FIG.1 Influence of Monoethyl amine / Monomethyl amine